

## Pressure Module (PM)

### ACCURACY

#### PSI (Gauge Pressure)

##### 30, 100, and 300 PSI modules

0 to 30% of Range:  $\pm(0.0075\%$  of Full Scale)

30 to 110% of Range:  $\pm(0.025\%$  of Reading)

Vacuum:  $\pm(0.06\%$  of Full Scale\*, typical)

\* Full Scale = -14.5 PSI

##### 1000 and 3000 PSI modules

0 to 30% of Range:  $\pm(0.015\%$  of Full Scale)

30 to 110% of Range:  $\pm(0.05\%$  of Reading)

##### 10 000 and 15 000 PSI modules

0 to 30% of Range:  $\pm(0.03\%$  of Full Scale)

30 to 110% of Range:  $\pm(0.1\%$  of Reading)

*Includes all effects of linearity, hysteresis, repeatability, temperature, and stability for one year.*

*All models indicate vacuum, but vacuum specification (typical) applies to 30, 100, and 300 PSI models only.*

*Not recommended for continuous use at high vacuum.*

*Refer to [XP2i-DP data sheet](#) for gauges that are intended for continuous high vacuum use.*

#### PSIA (Pressure with BARO module)

##### 30 PSI module

0.200 to 14.500 PSIA:  $\pm 0.011$  PSIA, typical

14.500 to 44.500 PSIA:  $\pm(0.025\%$  of Reading) + 0.003 PSIA

##### 100 PSI module

0.200 to 14.500 PSIA:  $\pm 0.011$  PSIA, typical

14.500 to 44.500 PSIA:  $\pm 0.011$  PSIA

44.500 to 114.500 PSIA:  $\pm(0.025\%$  of Reading)

##### 300 PSI module

0.20 to 14.50 PSIA:  $\pm 0.01$  PSIA, typical

14.50 to 104.50 PSIA:  $\pm 0.03$  PSIA

104.50 to 314.50 PSIA:  $\pm(0.025\%$  of Reading)

##### 1000 PSI module

14.5 to 314.5 PSIA:  $\pm 0.2$  PSIA

314.5 to 1014.5 PSIA:  $\pm(0.05\%$  of Reading)

##### 3000 PSI module

14.5 to 914.5 PSIA:  $\pm 0.5$  PSIA

914.5 to 3014.5 PSIA:  $\pm(0.05\%$  of Reading)

##### 10 000 PSI module


15 to 3015 PSIA:  $\pm 3$  PSIA

3015 to 10 015 PSIA:  $\pm(0.1\%$  of Reading)

##### 15 000 PSI module

15 to 4515 PSIA:  $\pm 5$  PSIA

4515 to 15 015 PSIA:  $\pm(0.1\%$  of Reading)

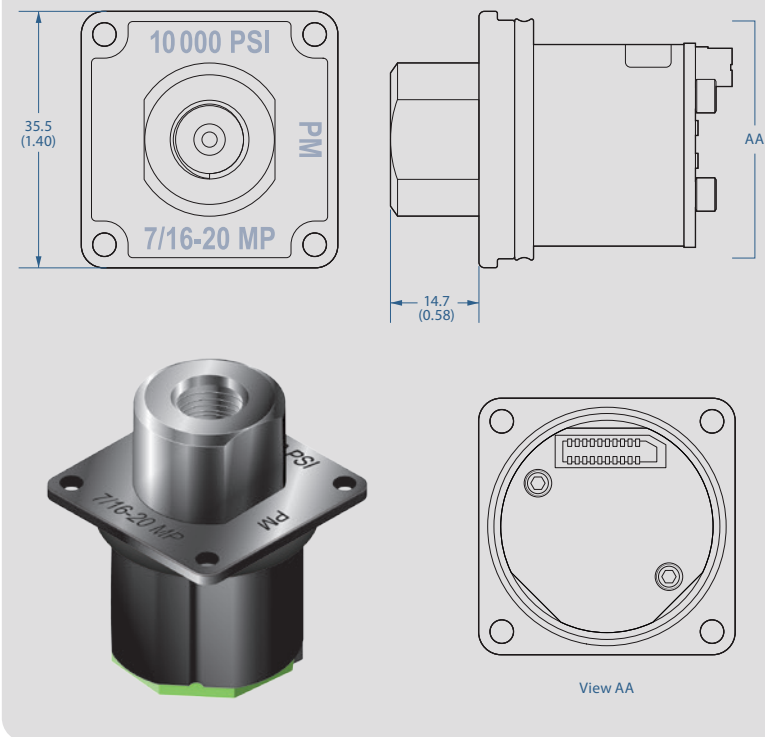

## DIFFERENTIAL PRESSURE MEASUREMENT UNCERTAINTIES WITH TARE

The Tare function can improve measurement uncertainties on two modules with the same full scale pressure range installed into one nVision Reference Recorder. Requires the use of an equalizing valve.

The following specifications apply to the measurement system with a logging interval of 1 second/reading:

Full Scale Range of Both Sensors	The Greater of (+/-)					% of DP Reading
	PSI	mbar	inH <sub>2</sub> O	mmH <sub>2</sub> O		
30	0.0005	0.04	0.014	0.4	or	0.025%
100	0.0015	0.10	0.04	1.0	or	0.025%
300	0.005	0.4	0.14	4.0	or	0.025%
1000	0.02	1.0	0.4	10.0	or	0.05%
3000	0.05	4.0	1.4	n/a	or	0.05%
10000	0.2	10.0	4.0	n/a	or	0.1%
15000	0.3	15.0	6.0	n/a	or	0.1%

Unit must be enabled in CrystalControl

## DIFFERENTIAL PRESSURE MEASUREMENT UNCERTAINTIES WITHOUT TARE

The total nVision Reference Calibrator measurement uncertainty in the  $\Delta P$  mode configuration will need to consider the uncertainties of both pressure modules. We recommend the module uncertainties to be combined with the preferred square root of the sum of the squares (or "root sum squares") method.

The following table lists the possible combinations of using Pressure Modules (PM) with different accuracy statements. The uncertainties reported below are without the use of the Tare feature, which will greatly improve your measurement uncertainty.

		Upper Pressure Module Uncertainties (of Static Line Pressure) (of Reading)		
		0.025%	0.05%	0.10%
Lower Pressure Module Uncertainties (of Static Line Pressure) (of Reading)	0.025%	0.035%	0.056%	0.103%
	0.05%	0.056%	0.071%	0.112%
	0.10%	0.103%	0.112%	0.141%

## SENSOR

Wetted Materials: (WRENCH TIGHT) **316 stainless steel**

(FINGER TIGHT) **316 stainless steel  
and Viton® (internal o-ring)**

Diaphragm Seal Fluid: **Dow Corning® 200**

Connection: **Crystal CPF Female**

*All welded, with a permanently filled diaphragm seal.*

*Metal to metal cone seal; O-ring can be removed if necessary.*

*1/4" medium pressure tube system compatible with HIP LM4 and LF4 Series, Autoclave Engr SF250CX Male and Female Series.*

*CPF Adapters to NPT, BSP, and M20 available.*

## BAROMETRIC REFERENCE (BARO)

Accuracy: **± 0.00725 PSI, ± 0.5 mbar**

Range: **10.153 to 15.954 PSIA,  
700.0 to 1100.0 mbarA**

Units and Resolution: **PSI ..... 0.001  
inHg ..... 0.001  
mmHg ..... 0.01  
mbar ..... 0.1**

Pressure Connection: **Cylindrical sensor fitting of 5.8mm  
OD. A flexible 4.8 mm [3/16"] ID  
tube is recommended to connect for  
for calibration.**

Mounting: **Secured using a 3/8" 4-40 plastic screw.**

*Includes all effects of linearity, hysteresis, repeatability,  
temperature, and stability for one year.*

*Exposure to environmental extremes of temperature, shock, and/  
or vibration may warrant a more frequent recertification period.*

*Other units available depending on the installed modules.*



## Current, Voltage, & Switch Test Module (MA20)

Intended for use with a 4-20mA loop measurement. This module is also capable of measuring supply voltages and has an auxiliary fixed output for use in switch open/closure testing. Each MA20 module includes a super flexible silicone test lead kit (P/N 3952).

### CURRENT & VOLTAGE MEASUREMENT

#### Current (mA) Input

Accuracy:  $\pm(0.015\% \text{ of rdg} + 0.002 \text{ mA})$

Range: **0 to 55 mA (MA20+)**  
**0 to 25 mA (MA20)**

Max Allowable Current: **93.3 mA**

Resolution: **0.001 mA or 0.01%**

Units: **mA, % 4-20, % 10-50**

Input Resistance: **< 17.2  $\Omega$**

Voltage Burden @ 20mA: **< 0.35 V**

Voltage Burden @ 50mA: **< 0.86 V**

HART Resistance: **250  $\Omega$**

Connection: **2mm jacks**

*Includes all effects of linearity, hysteresis, repeatability, temperature, and stability for one year.*

**WARNING:** ATEX and IECEx certification does not allow the installation of two MA20 modules.

*Inputs protected by a resettable fuse.*

*mA can be displayed as a percentage, where 0 to 100% corresponds to either 4 to 20 mA or 10 to 50 mA.*

*Jacks are compatible with safety sheathed banana plugs.*

#### Voltage (VDC) Input

Accuracy:  $\pm(0.015\% \text{ of rdg} + 0.002 \text{ VDC})$

Range: **0 to 28 VDC**

Max Allowable Voltage: **30 VDC**

Resolution: **0.001 VDC**

Units: **VDC**

*Includes all effects of linearity, hysteresis, repeatability, temperature, and stability for one year.*

#### Switch Test


Switch Type: **Dry Contact**

Closed State Resistance: **< 10  $\Omega$**

Open State Resistance: **> 10 M $\Omega$**

*Switch state change indicated by bright green LED flash.*

*Switch test screen reports switch open, close, and deadband values.*

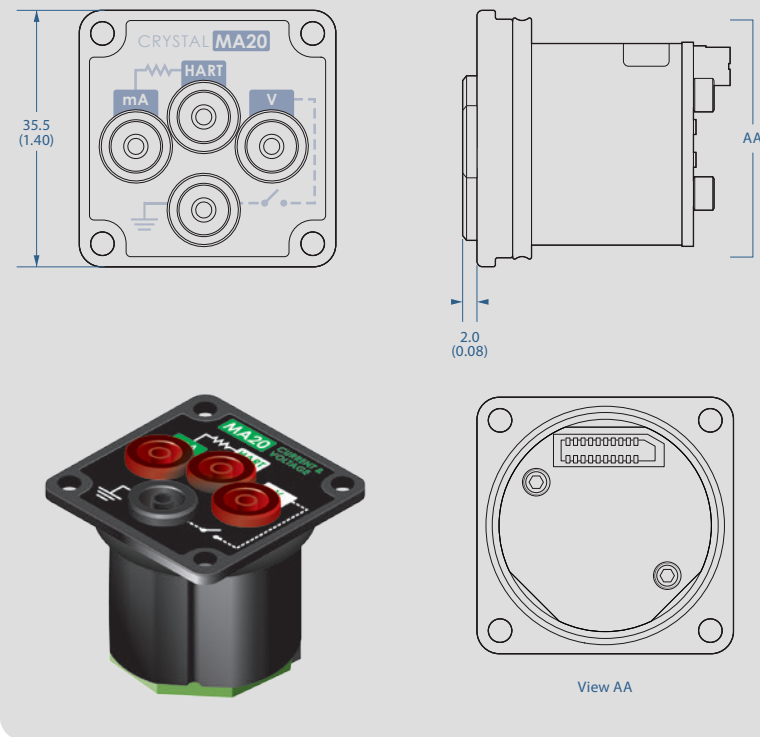

#### ATEX and IECEx Scheme Entity Parameters

The MA20 Module has these specific input entity parameters:

**Ui = 28 V**

**Uo = 6.6 V**

**Ii = 93.3 mA**

**Io = 4.45 mA**

**Pi = 653.3 mW**

**Po = 7.34 mW**

**Ci = 0.36  $\mu$ F**

**Co = 0.5  $\mu$ F\***

**Li = 39.1  $\mu$ H**

**Lo = 12  $\mu$ H\*\***

\* Dependent on the supply to the terminals but shall not be greater than 0.5  $\mu$ F

\*\* Total cable inductance between all modules

## Temperature Module (RTD100)

Calibrated for Pt100 RTD/PRT (100 Ohms at 0°C Platinum Resistance Temperature Detector) sensors conforming to DIN/IEC 60751 (or IEC751) with US, Euro, or Lab calibration curves. An RTD is not included, but each RTD100 includes P/N 3953 RTD Connection Kit.

### TEMPERATURE MEASUREMENT

#### Resistance Input

Accuracy:  $\pm (0.015\% \text{ of rdg} + 0.02 \Omega)$

Range: **0 – 400 Ohms range for use with 100 Ohm PRTs**

Resolution: **0.01 on all scales**

Units: °C, K, °F, R,  $\Omega$

TCRs: **0.003850  $\Omega/\Omega/^\circ\text{C}$  (IEC 60751), 0.003911  $\Omega/\Omega/^\circ\text{C}$  (US Industrial Std), 0.003926  $\Omega/\Omega/^\circ\text{C}$**


Wiring: **2-, 3-, 4-wire support**

Connection: **M8 connector cable or terminal block**

*Includes all effects of linearity, hysteresis, repeatability, temperature, and stability for one year.*

The proper selection of the RTD sensing element is very important as the error associated with this device is the majority of the overall system measurement uncertainty. IEC 751 is the standard that defines the temperature versus resistance for 100 $\Omega$ , 0.00385  $\Omega/\Omega/^\circ\text{C}$  platinum RTDs. IEC 751 defines two classes of RTDs: Class A and B. Class A RTDs operate over the -200 to 630°C range versus -200 to 800°C for the Class B elements. For example, the Class A uncertainty is about half that of the Class B elements as illustrated in the following table.

Temperature	nVision Uncertainty		Class A				Class B			
			Class A Uncertainty		nVision + Class A Uncertainty		Class B Uncertainty		nVision + Class B Uncertainty	
			$\pm\Omega$	$\pm^\circ\text{C}$	$\pm\Omega$	$\pm^\circ\text{C}$	$\pm\Omega$	$\pm^\circ\text{C}$	$\pm\Omega$	$\pm^\circ\text{C}$
-200	$\pm\Omega$	0.05	0.02	0.05	0.24	0.55	0.24	0.55	0.56	1.30
0	0.04	0.09	0.06	0.15	0.07	0.17	0.12	0.30	0.12	0.31
200	0.05	0.13	0.2	0.55	0.21	0.56	0.48	1.30	0.48	1.31
400	0.06	0.17	0.33	0.95	0.33	0.96	0.79	2.30	0.79	2.31
600	0.07	0.21	0.43	1.35	0.44	1.37	1.06	3.30	1.06	3.31
800	0.08	0.25	0.52	1.75	0.53	1.77	1.28	4.30	1.28	4.31

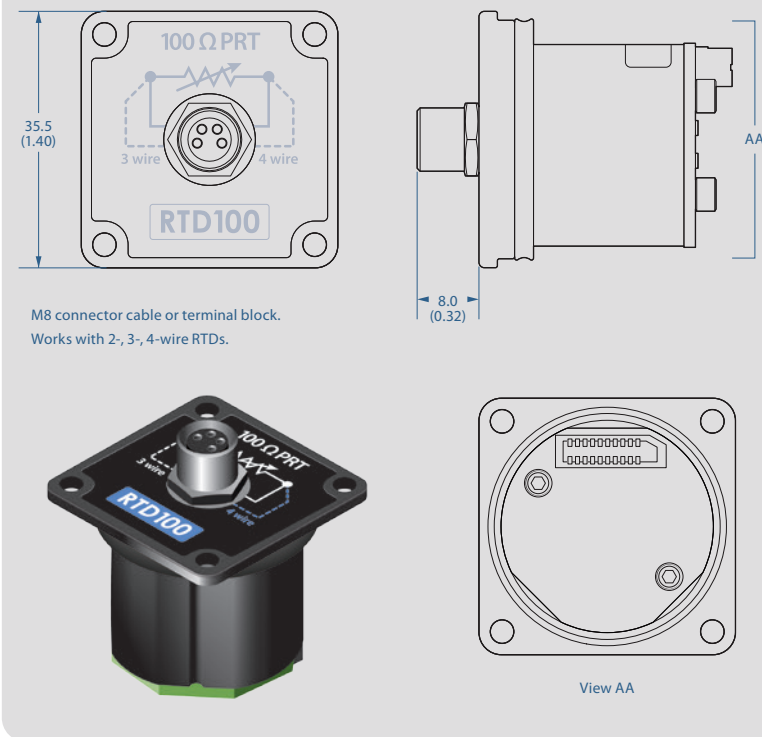

M8 connector cable or terminal block.  
Works with 2-, 3-, 4-wire RTDs.

View AA



#### ATEX and IECEx Scheme Entity Parameters

The RTD100 Module has these specific input entity parameters:

$U_i = 0 \text{ V}$

$I_i = 0 \text{ A}$

$P_i = 0 \text{ W}$

$U_o = 9.73 \text{ V}$

$I_o = 1.6642 \text{ A}$

$P_o = 1.1 \text{ W}$

$C_o = 0.5 \mu\text{F}$

$L_o = 12 \mu\text{H}^*$

\* Total cable inductance between all modules

## nVision Chassis (NV)

### OPERATING TEMPERATURE

Temperature Range: **-20 to 50° C (-4 to 122° F)**

< 95% RH, non-condensing. No change in accuracy over operating temperature range. Gauge must be zeroed to achieve rated specification.

Applies to all modules.

### DISPLAY

Screen: **255 x 160 pixel graphical display**

LCD readable in sunlight with bright backlight.

Display Rate: **4 readings/second (standard)**  
**up to 10 readings/second (recording)**

### POWER

4 x AA: **200 hours, typical**

Ultra Low Power: **Up to 60 days, typical\***

Approved Batteries: **The nVision is Intrinsically Safe only if powered by one of the following battery types:**

Approved Battery Type	Ta=	Marking
Rayovac Max Plus 815	-20 to 50° C	Ex ia IIB T4 Ga
Duracell MN1500	-20 to 45° C	
<b>**Energizer E91, EN91</b>	-20 to 50° C	Ex ia IIB T3 Ga
Duracell MN1500		

\*2 installed modules, 1 reading per 5 minute recording interval, and 23° C ambient temperature.

**WARNING:** Do not use the mini-USB serial interface in hazardous locations.

**WARNING:** Replace batteries with approved type in non-hazardous locations only.

Uses 4 alkaline AA (LR6) batteries. Use of backlight reduces operating time.


**\*\*Energizer is manufactured by Energizer Holdings, Inc., and the Eveready Battery Company, Inc.**

### DATA/COMMUNICATION

Digital Interface: **mini-USB**

The mini USB will power the nVision with or without the battery pack installed.

**WARNING:** Do not use the mini-USB serial interface in hazardous locations.

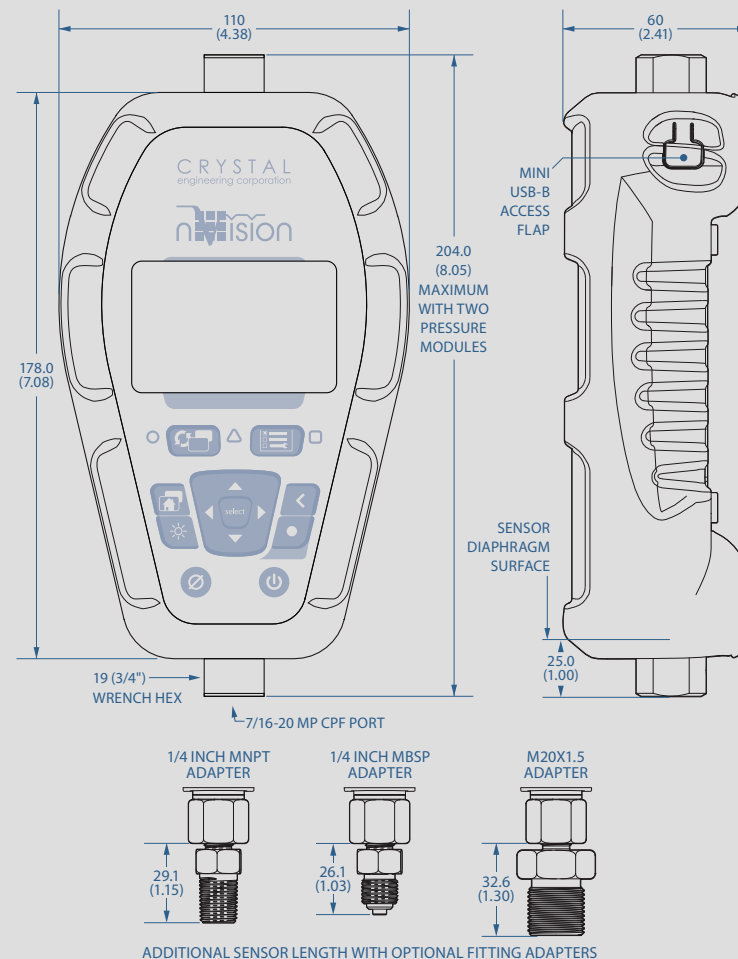

## DATALOGGING

Capacity: **Approx. 1,000,000 data points\***

Storage Type: **Non-volatile flash memory**

Fastest Interval: **10 per second**

Slowest Interval: **1 per hour**

*\*Single Module Recording*

*The included CrystalControl software is compatible with 32 & 64 bit Windows 7 and Vista, and XP (32 bit only). Produces csv, xls, pdf, or signed pdf files, and uses Excel template files (samples included) to automatically format and graph data.*

## ENCLOSURE

Weight: **680 g (24.0 oz)**

Rating: **IP67**

Housing: **Impact resistant injection molded**

Keypad and Labels: **UV Resistant Polyester**


Mounting: **M4 x 0.7 [8 mm (0.31")] deep threaded insert mounting locations**

*Weight includes one pressure module, one RTD module, 4AA battery module, and protective boot.*

*Submersible to 1 m for 30 minutes [IEC 60529].*

*LCD protected from impact damage by 1.5 mm (0.06") thick polycarbonate lens.*

*Skydrol® compatible.*

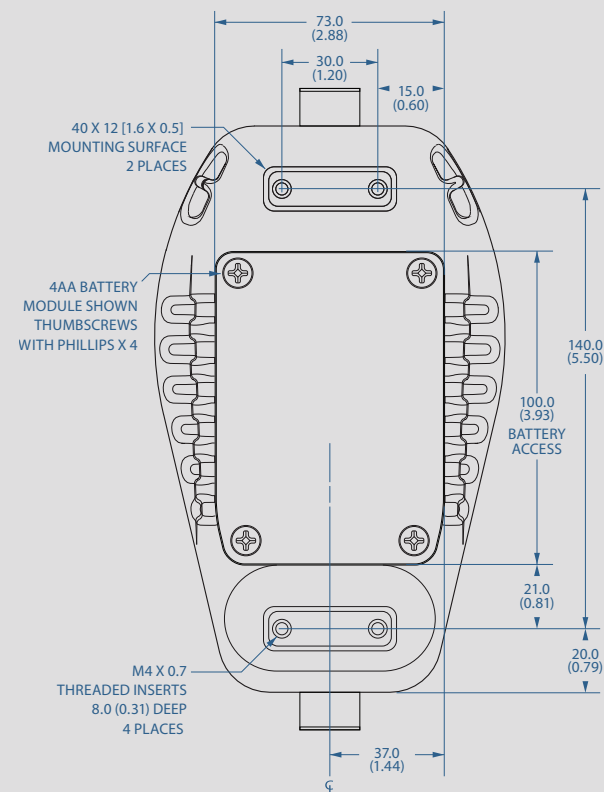

## STORAGE TEMPERATURE

Temperature Range: **-40 to 75° C (-40 to 167° F)**

*Batteries should be removed if stored for more than one month.*

## SPECIAL FEATURES

The following requires the use of our free CrystalControl software

Averaging Screen: **Averages all points in a recording run.**

Data Point Counter: **Screen for counting the data points logged.**

Display Screens: **Turn on and rearrange display screens.**

Estimated Recording Time: **A CrystalControl calculation based on active screens and logging interval.**

Live PC Graph: **During a recording, graph directly to your PC.**

Password Protect: **Changes to configuration or userspan calibration factor(s).**

Pressure Switch Test: **Using a PM and MA20, get deadband and state-change pressure.**

Remove: **Unwanted pressure units.**

Run Tags: **Create and enable run tags that will identify logging runs.**

Screen Numbers: **Number each display screen to make writing procedures around the nVision easier.**

Secure Documents: **Download into secure pdf documents for tamper proof records.**

Start-up Screen: **Define a 32-character prompt which requires user acknowledgement at startup.**

User Defined Unit: **Define and display any pressure units not included, or to use the gauge to display force, level or other pressure related parameters.**

## CERTIFICATIONS



**II 1G Ex ia IIB T4 Ga or T3**  
**SIRA 09ATEX2008X**

This product conforms to:

**EN 60079-0: 2006 | EN 60079-11: 2007 | EN 60079-26: 2007**



**Ex ia IIB T4 Ga or T3**  
**IECEX SIR09.0053X**

This product conforms to:

**IEC 60079-0: 2004 | IEC 60079-11: 2006 | IEC 60079-26: 2006**



nVision complies with the Electromagnetic Compatibility and the Pressure Equipment Directives. Refer to the EC Declaration of Conformity for specific details.



The instrument was tested against **AS/NZS 3584**, C-tick EMC/EMI requirements.



XP2i is approved for use as a portable test instrument for Marine use and complies with Det Norsjke Veritas' Rules for Classification of Ships, High Speed & Light Craft and Offshore Standards.

## RANGE & RESOLUTION TABLE

PM	Range (PSI)	Over-pressure	Display Resolution									
			PSI	in H <sub>2</sub> O	in Hg	mm Hg	mm H <sub>2</sub> O	kg/cm <sup>2</sup>	bar	mbar	kPa	MPa
30PSI	30	3.0 x	0.001	0.01	0.001	0.01	1	0.0001	0.0001	0.1	0.01	
100PSI	100	2.0 x	0.001	0.1	0.01	0.1	1	0.0001	0.0001	0.1	0.01	0.00001
300PSI	300	2.0 x	0.01	0.1	0.01	0.1		0.001	0.001	1	0.1	0.0001
1KPSI	1000	2.0 x	0.1		0.1			0.001	0.001		0.1	0.0001
3KPSI	3000	1.5 x	0.1		0.1			0.01	0.01		1	0.001
10KPSI	10 000	1.5 x	1					0.01	0.01		1	0.001
15KPSI	15 000	1.3 x	1					0.01	0.01		1	0.001

Add one digit of resolution for differential mode.

## ORDERING INFORMATION

Product ID	Power	Module: Upper	Module: Lower	BARO Module?
NV	4AA	—	—	—
		PM	PM	No: (omit)
		MA20	MA20	Yes: -BARO
		RTD100	RTD100	
		BNKPLT	BNKPLT	

If ordering a nVision with only one module installed, please enter "BNKPLT" in the empty module slot.

## SAMPLE PART NUMBERS

NV-4AA-30PSI-3KPSI-BARO ... nVision with 30 PSI pressure module (upper) and 3000 PSI pressure module (lower) with BARO module option

NV-4AA-RTD100-10KPSI ... nVision with RTD100 temperature module (upper) and 10 000 PSI pressure module (lower)

## ACCESSORIES (Included with NV)

### Soft Carrying Case P/N 4087

Durable, padded case with separate pockets for your nVision and accessories.

### Protective Boot P/N 3985

Shock resistant protection, low durometer, Skydrol resistant.

### Mini-USB Cable P/N 3951

Connect to your nVision with 6' [1.8m] cable.

## COMPLIMENTARY PRODUCTS

**Crystal Engineering offers a wide range of products that work with the nVision:**

- [Fittings that connect without tools, safely and without leaks](#)
- [Lightweight, super flexible high pressure hoses](#)
- [Fitting kits and adapters](#)
- [Pneumatic hand pumps](#)
- [Hydraulic hand pumps](#)
- [Portable pressure comparators](#)
- [Software, for the quickest way to calibrate pressure transmitters and gauges](#)

Dow Corning is a registered trademark of Dow Corning Corporation.